

Simplified LC-MS/MS Method for Glyphosate, AMPA, and Glufosinate in oat-based cereals

Olga I. Shimelis, R&D Manager; Teresa Marsala, Senior R&D Technician; M. James Ross, Senior R&D Scientist, analytix@merckgroup.com

Summary

A LC-MS/MS method with simple SPE interference removal for the determination of glyphosate, (aminomethyl)phosphonic acid (AMPA), and glufosinate in cereals is described. A carbon-based chromatography column allowed retention of the analytes while ammonium carbonate mobile phase system insured proper ionization under negative ESI conditions.

Abstract

A simplified LC-MS/MS method for the determination of glyphosate, (aminomethyl) phosphonic acid (AMPA), and glufosinate in cereals is described. The method enables the analysis of glyphosate and its metabolites without sample derivatization. The samples are prepared utilizing an extraction method based upon the Quick Polar Pesticides (QuPPE) Method and separated by high-performance liquid chromatography with MS detection. A carbon-based chromatography column allowed retention of the analytes while water, methanol and ammonium carbonate mobile phase system insured proper ionization under negative ESI conditions. The use of a sensitive Sciex 6500 MS instrument enabled low detection limits of 10 ppb in oats-based samples to be attained. Multiple cereals were analyzed and incurred levels of glyphosate, AMPA and glufosinate were found to be above the detection limits of the method.

Key Words

Glyphosate, AMPA, glufosinate, cereal, grain, LC-MS/MS, pesticides, food

Introduction

Glyphosate is one of the most used herbicides in the world with more than 1.4 billion pounds of glyphosate applied to fields per year.¹ This chemical's usage increased after the introduction of genetically modified, glyphosate tolerant crops such as corn, soybeans, and cotton. In the USA, US Environmental Protection Agency (EPA) regulation document Code of Federal Regulations (CFR)-title 40-volume 26 sets the tolerance levels for the occurrence of glyphosate in food commodities and produce.² The EPA tolerance for glyphosate residues in cereal grains (also called crop group 15) are set at 30 ppm; this limit excludes rice, soy, and corn. In rice, the tolerance is 0.1 ppm whereas, in sweet corn it is 3.5 ppm.² For glufosinate, an herbicide that is often included with glyphosate in analytical methods, the tolerance values are 0.4 ppm for cereal and 1.0 ppm for rice. These tolerance values include metabolites and degradants. Therefore, a glyphosate metabolite, AMPA, was also included into this study (**Figure 1**). For comparison, in the European Union (EU) maximum residue levels (MRL) in oats are 20 mg/kg for glyphosate and 0.03 mg/kg for

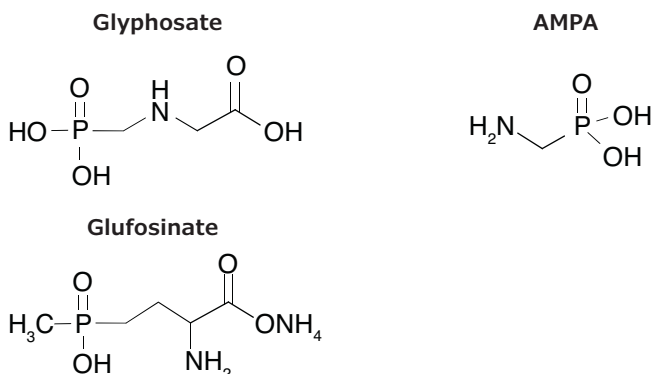


Figure 1. Structures of Glyphosate, AMPA and Glufosinate

Glufosinate (lower limit of analytical detection) and for glyphosate in rice MRL is 0.03 mg/kg (lower limit of analytical detection) and for glufosinate 0.9 mg/kg.³

In this application, the presence of glyphosate in cereal grains, and oat, in particular, used in the production of breakfast cereals, was explored.

Various methods for glyphosate analysis were developed over the last 30 years. Some methods required derivatization of analytes for HPLC analysis, with fluorescence detection, with o-phthalaldehyde.⁴ A method with glyphosate derivatization using fluorenylmethyloxycarbonyl chloride (FMOC) and

fluorescence detection has also been proposed and widely used.⁵ Recently, with the advent of modern, sensitive, and rugged LC-MS/MS instruments, it has become possible to analyze glyphosate and its metabolites without derivatization as illustrated in this work with direct analysis of glyphosate by MS/MS. Multiple columns were previously used for mass spectrometry-based glyphosate analysis including ion-exchange, hydrophilic interaction liquid chromatography (HILIC), or carbon HPLC columns.⁶ Some of the HILIC-based and ion-exchange methods used positive ESI for detection of glyphosate and analogues and acidic mobile phases.^{6,7} The HILIC-based methods present a challenge of solvating these very polar analytes in the non-polar diluent. Ion-exchange methods utilized negative ionization mode for detection and citric acid or citric salts in the mobile phase⁵ which are not volatile and therefore not fully compatible with mass spectrometric detection. We have shown previously that detection of glyphosate in negative ESI was possible using carbonate buffer and an anion exchange column.⁸ In this work, we used a volatile bicarbonate buffer mobile phase and a Supel™ Carbon LC U/HPLC column. This column possesses a unique mixed-mode retention mechanism that allows better retention of polar analytes.

Experimental

Glyphosate, AMPA and ammonium glufosinate were of analytical standard grade. Isotopically labelled internal standards were used including glyphosate-2-¹³C, ¹⁵N, AMPA-¹³C, ¹⁵N, and glufosinate-D₃. Solutions of internal standards and non-isotopically labelled standards were prepared in water at 1 mg/mL and used for spiking the grain matrices.

Organic oatmeal was selected as test matrix and used during method development. Multiple samples of organic oatmeal from local stores were scanned for the presence of glyphosate using the methods described below. All oatmeals had some level of glyphosate and other compounds present. For the method development study, a cereal sample was selected that had the lowest overall background for all three analytes containing only glyphosate at 24 ppb. This specific matrix was spiked to contain either 80ppb and 800ppb of all 3 analytes. The spiked samples were used to evaluate the recovery of analytes during method development and for validation.

Additionally, multiple samples of oat cereals were purchased in the local grocery store and evaluated for glyphosate contamination using the developed method (**Figure 2**)

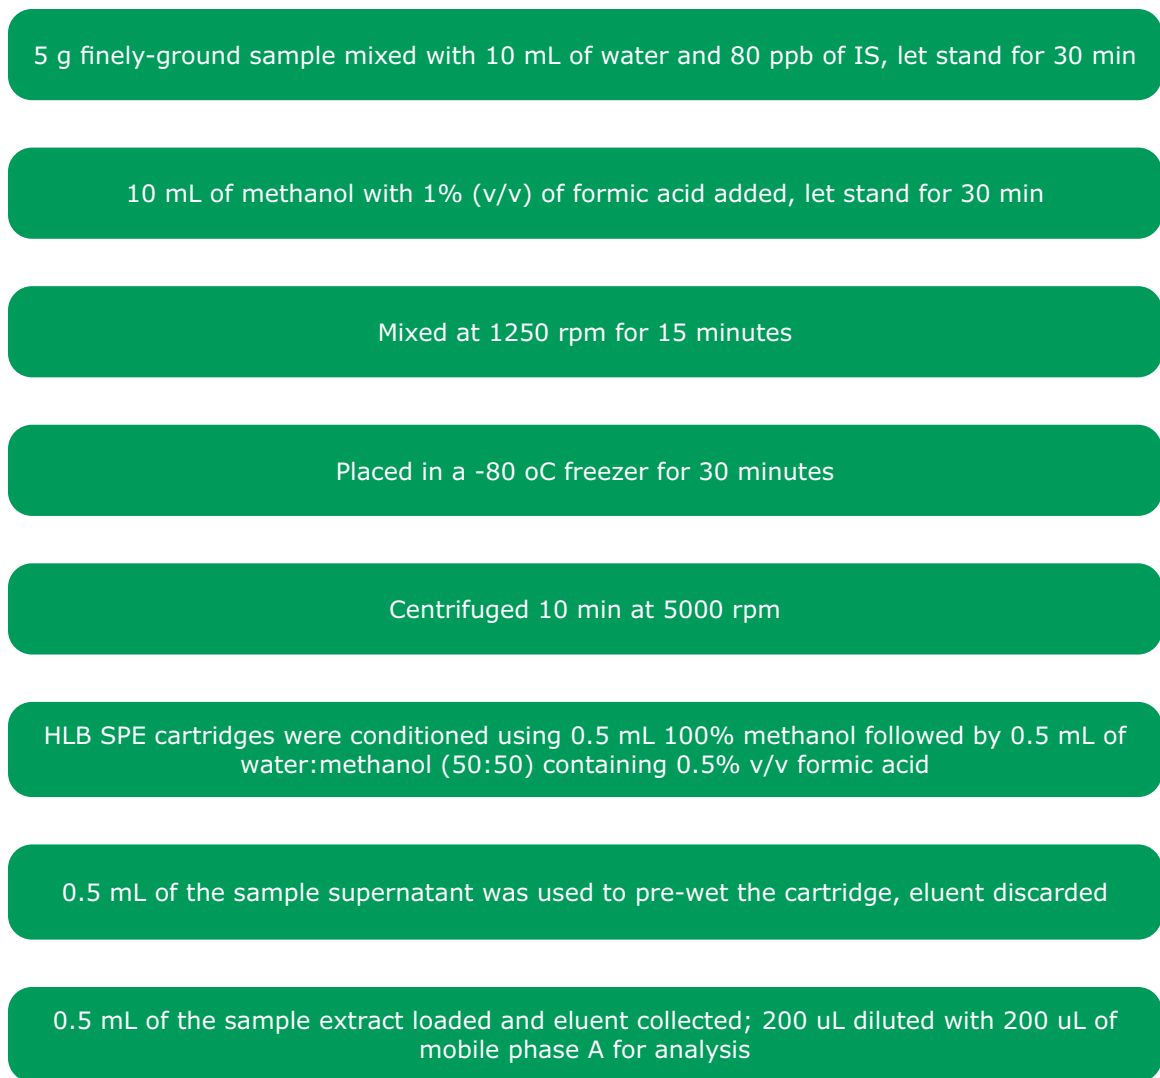


Figure 2. Sample preparation method

Sample preparation

The extraction method was based on the QuPPe (Quick Polar Pesticides Method) methodology developed in the European Union (EU) for fruits and vegetables, and used water: methanol (50:50) containing 0.5% formic acid (V/V) as the final extraction solvent.⁶

Solid phase extraction (SPE) cleanup using Supel™ Swift HLB cartridges was applied to the extract, similarly to a method reported by Chamkasem and Harmon.⁹ Hydrophilic-lipophilic balance, or HLB, SPE can be applied to a broad range of analytes using reversed phase methodology. The SPE cleanup method in the present work is based on the chemical “filtration” (interference removal) of the extract through the HLB cartridge when the impurities that are more hydrophobic in comparison to the analytes are retained on the SPE phase while the more polar analytes do not retain and come through in the eluate


LC-MS/MS method

The analysis was completed using a Supel™ Carbon LC U/HPLC column, which provided good retention for these polar analytes. The aqueous mobile phase [A] used was an ammonium carbonate buffer, pH 9. This mobile phase ensured the proper ionization of the phosphate or phosphonate moiety in the analytes (**Figure 1**) monitored under negative ESI conditions. In addition, ammonium carbonate buffer is volatile and is fully compatible with LC/MS instrumentation. The organic mobile phase [B] contained acetonitrile: water (95:5). The method operated under both a mobile phase and a flow rate gradient. **Table 1** lists the MS analyte parameters. **Figure 3** presents a chromatogram of a standard injection and LC instrument parameters.


Solvent-based external calibration curves used internal standards and were prepared in 75:25 water: methanol with 0.25% (v/v) formic acid. The concentration range of calibration curves was from 1 ng/mL to 150 ng/mL and the linearity was better than R² of 0.998. Representative calibration curve for glyphosate is shown in **Figure 4**.

Table 1. MS parameters for analytes

Compound		Q1	Q3	DP	EP	CX
Glyphosate	Quant	168	63	-30	-5.9	-26
	Qual	168	124	-30	-5.5	-16
glyphoste-2- ¹³ C	Quant	167	63	-30	-6.5	-28
	Qual	110	80	-15	-10.0	-36
AMPA	Quant	110	63	-15	-10.0	-28
	Qual	110	80	-15	-10.0	-36
AMPA- ¹³ C	Quant	112	63	-15	-6.5	-24
	Qual	180	63	-50	-6.0	-56
Glufosinate	Quant	180	63	-50	-6.0	-56
	Qual	180	95	-50	-10.0	-24
Glufosinate-D ₃	Quant	183	63	-50	-5.0	-70
	Qual	183	63	-50	-5.0	-70

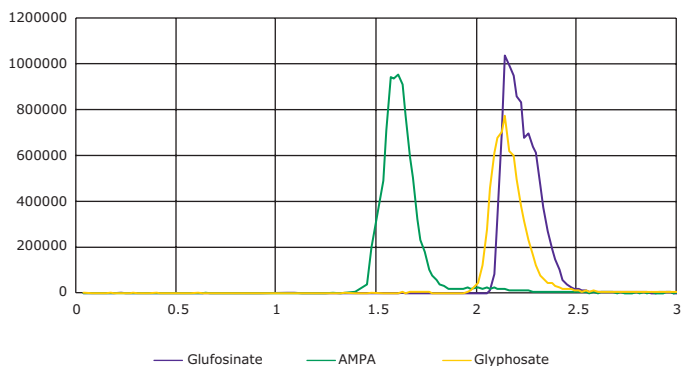**Figure 3.** LC/MS Analysis of Glyphosate, AMPA, and Glufosinate using Supel™ Carbon HPLC column. Quantitative transitions are shown for each analyte. Conditions are described in the experimental section. 100 ng/mL calibration standard is shown.

LC Conditions																							
Instrument:	Agilent 1290 HPLC with AB Sciex Triple Quad 6500																						
Columns:	Supel™ Carbon LC, 10 cm x 2.1 mm, 2.7 μm (59986-U)																						
Mobile phase:	[A] 20mM ammonium carbonate pH; [B] acetonitrile:water (95:5)																						
Gradient:	<table><tr><th>Time (min)</th><th>A (%)</th><th>B (%)</th></tr><tr><td>0</td><td>100</td><td>0</td></tr><tr><td>3.0</td><td>100</td><td>0</td></tr><tr><td>3.1</td><td>0</td><td>100</td></tr><tr><td>5.0</td><td>0</td><td>100</td></tr><tr><td>5.1</td><td>100</td><td>0</td></tr><tr><td>8.0</td><td>100</td><td>0</td></tr></table>		Time (min)	A (%)	B (%)	0	100	0	3.0	100	0	3.1	0	100	5.0	0	100	5.1	100	0	8.0	100	0
	Time (min)	A (%)	B (%)																				
	0	100	0																				
	3.0	100	0																				
	3.1	0	100																				
	5.0	0	100																				
	5.1	100	0																				
	8.0	100	0																				
Flow:	<table><tr><th>Flow rate (mL/min)</th></tr><tr><td>0.2</td></tr><tr><td>0.2</td></tr><tr><td>0.5</td></tr><tr><td>0.5</td></tr><tr><td>0.2</td></tr><tr><td>0.2</td></tr></table>		Flow rate (mL/min)	0.2	0.2	0.5	0.5	0.2	0.2														
	Flow rate (mL/min)																						
	0.2																						
	0.2																						
	0.5																						
	0.5																						
	0.2																						
0.2																							
Column Temp.:	30 °C																						
Detection:	ESI (-) MS/MS (See Table 1)																						
Injection:	20 μL																						
MS Parameters																							
Voltage:	-4500 V																						
Curtain gas:	30																						
Source temp:	600 °C																						
Gas 1 / Gas 2:	50 / 70																						

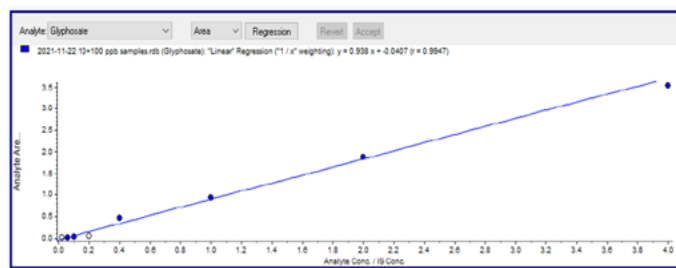**Figure 4.** Representative calibration curve for glyphosate

Results

Method development

Sample preparation used fast solvent extraction. SPE was the first choice for sample cleanup as the sample can be simply passed through the cartridge. As all analytes in this method are polar, they were not retained on the reversed-phase SPE and were passed through and expected to achieve good recoveries.

The chosen chromatographic method allowed the injection of the prepared extract after a dilution step which resulted in a convenient and fast analysis method. The elution off the HPLC column was performed isocratically using aqueous carbonate buffer as the mobile phase. A column wash step followed using acetonitrile. Multiple injections ($n > 100$) of extracted samples did not result in significant retention time change. For example, the retention time variability across 5 days of injections and two different mobile phases preparations had RSD of 3.2% indicating the ruggedness of this LC method.

Organic oatmeal samples were screened for glyphosate and related compounds. These results are shown in **Table 2**. All compounds were found to be present in all samples indicating the good sensitivity of the proposed method. The sample with the lowest overall concentration for incurred analytes, Sample N, was chosen to be used for method validation.

Six replicates of the Sample N were spiked with 24 ppb to determine the method's limit of quantitation (LOQ) for all three analytes. The recoveries were found to be

Table 2. Background analysis results for organic oat cereals

Cereal	glyphosate (ppb)	AMPA (ppb)	Glufosinate (ppb)
Sample S	8.0	38	44
Sample Z	4.8	198	39
Sample N	24.6	ND	ND
Water control	ND	ND	ND

within 80-120% with an RSD of below 15%. The LOQ was determined at the signal-to-noise ratio of 10:1 for glyphosate as 6 ppb, for AMPA – 11 ppb, and for glufosinate – 8 ppb.

Sample N was spiked with the three analytes at both 80 ppb and 800 ppb levels. Glyphosate and AMPA chromatograms for the 800 ppb spiked sample are shown in **Figure 5**. The quantitation results are shown in **Table 3**. All three analytes were detected and quantified at both spiking levels. Accuracy of the method was measured as the percent recovery of the known spiked amounts. For 80 ppb and 800 ppb spikes, the recovery values for glyphosate were 124% and 96%, for glufosinate, they were 132% and 104%, and for AMPA the recoveries were at 80% and 88% respectively on day one. Similar recoveries were achieved on the second day of testing when

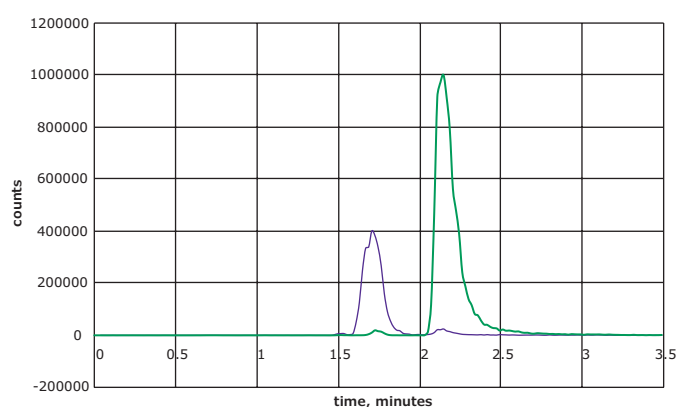


Figure 5. Glyphosate (red trace) and AMPA (blue trace) spiked into oatmeal at 800 ppb

Table 3. Method validation results after spiking 80 ppb and 800 ppb into cereal/grains labelled “organic”

Spiking level (n=5)	Compound	Day 1 % recovery (%RSD)	Day 2 % recovery (%RSD)
80 ppb	Glyphosate	124 (6)	134 (7)
	AMPA	132 (6)	106 (13)
	Glufosinate	80 (18)	109 (6)
800 ppb	Glyphosate	96 (3)	96 (4)
	AMPA	104 (10)	91 (7)
	Glufosinate	89 (4)	111 (5)

the samples were extracted and analyzed again. Reproducibility of the method was excellent with below 10% RSD for 800 ppb spiked samples and below 20% RSD for 80 ppb spiked samples.

Identification and quantitation of glyphosate in cereals

The results of glyphosate analysis in cereals using the proposed method are presented in **Table 4**. These samples were purchased in the grocery store, sample N was labelled “organic”. Internal standards were used as described in the experimental section. The samples were found to contain 25-260 ppb of glyphosate. AMPA levels in oat-containing samples varied from non-detected to 40 ppb. Glufosinate levels were found to be below LOQ.

Conclusion

Table 4. Results of analysis for oat-containing cereals

Samples n=3	Glyphosate (ppb)	% RSD	AMPA (ppb)	%RSD	Glufosinate (ppb)	% RSD
Sample N	24.6	5.0	ND	n/a	ND	5.4
Sample C	178.0	3.0	12	1.4	5.6*	6.9
Sample R	259.0	9.7	41	9.9	5.0*	3.5

* Below determined LOQ

The developed method for glyphosate and related compounds uses LC-MS/MS detection and a Supel™ Carbon LC U/HPLC column that is stable under higher pH conditions and provided sufficient retention for the polar analytes in the presence of methanol as extraction solvent. The mobile phase used 20 mM carbonate buffer being fully compatible with mass spectrometry and allowing for an efficient ionization. For the oat cereal samples, the extraction was based on the QuPpe method using a mixture of methanol and water followed by a cleanup using polymeric Supel™ Swift HLB SPE. The use of stable isotopic labelled internal standards resulted in good accuracy for glyphosate and related compounds. Further, it allowed the use of solvent-based calibration curves. The lower limit of quantitation (LOQ) for glyphosate for this method using a triple-quad MS detection was determined at 6 ppb. The analyzed samples of oat-containing cereals were found to contain 25-260 ppb of glyphosate.

References

1. Grossmann E., What Do We Really Know About Roundup Weed Killer?; National Geographic Apr 23, 2015, <http://news.nationalgeographic.com/2015/04/150422-glyphosate-roundup-herbicide-weeds/> (accessed December 17, 2021).
2. Glyphosate; tolerances for residues. § 180.364 <https://www.govinfo.gov/app/details/CFR-2020-title40-vol26/CFR-2020-title40-vol26-sec180-364> (accessed January 14, 2022).
3. European commission EU pesticide database, pesticide residue(s) and maximum residue levels (mg/kg) https://ec.europa.eu/food/plant/pesticides/eu-pesticides-database/mrls/?event=details&pest_res_ids=120,320&product_ids=236,237&v=1&e=search.pr (assessed January 12, 2022)
4. Methods for the Determination of Organic Compounds in Drinking Water- Supplement I (EPA/600/4-90-020). This document is available through NTIS (<http://www.ntis.gov>). https://www.nemi.gov/methods/method_summary/4806/ (accessed January 25, 2022).
5. Ehling, S.; Reddy, T.M. Total Residue Analysis of Glyphosate and Three Metabolites in Soy and Milk-based Nutritional Ingredients by Derivatization with Fluorenylmethyloxycarbonyl Chloride and Liquid Chromatography/Mass Spectrometry. Poster in Proceedings of ASMS, San Antonio, TX, 2016EURL-SRM
6. Quick Method for the Analysis of Highly Polar Pesticides in Food Involving Extraction with Acidified Methanol and LC- or IC-MS/MS Measurement Quick Polar Pesticides Method, I. Food of Plant Origin (QuPPE-PO-Method), Version 12, https://www.eurl-pesticides.eu/userfiles/file/EurlSRM/EurlSrm_meth_QuPPE_PO_V12.pdf (accessed December 17, 2021)
7. Nagatomi, Y., et al. Simultaneous LC-MS/MS Analysis of Glyphosate, Glufosinate, and Their Metabolic Products in Beer, Barley Tea, and Their Ingredients, BioSci. Biotechnol. Biochem., 2013, 77 (11), 2218–2221. DOI: 10.1271/bbb.130433
8. Shimelis O., LC-MS/MS Method for Determination of Glyphosate, AMPA, and Glufosinate in Cereals; Chromatography Today, Jun 12 2019, <https://www.chromatographytoday.com/article/lc-ms/48/milliporesigma/lc-msms-method-for-determination-of-glyphosate-ampa-and-glufosinate-in-cereals/2556> (accessed Dec 22, 2021)
9. Chamkasem., N.; Harmon, T. Direct determination of glyphosate, glufosinate, and AMPA in soybean and corn by liquid chromatography/tandem mass spectrometry. Anal. Bioanal. Chem. 2016, 408(18), 4995-5004. DOI: 10.1007/s00216-016-9597-6

Featured Products

Name	Cat. No.
HPLC & SPE	
Supel™ Carbon LC, 10 cm x 2.1 mm, 2.7 µm	59986-U
Supel™ Swift HLB SPE Tubes, 30 mg/1 mL, Pk. 108	57493-U
Reference Materials	
Aminomethylphosphonic acid (AMPA), analytical standard PESTANAL®, 50 mg	05164
Glyphosate, analytical standard PESTANAL®, 250 mg	45521
Glufosinate-ammonium, analytical standard PESTANAL®, 100 mg	45520
Glyphosate-2-13C,15N, analytical standard PESTANAL®, 5 mg	90479
Solvents, Reagents & Accessories	
Acetonitrile hypergrade for LC-MS LiChrosolv®	1.00029
Methanol UHPLC, suitable for mass spectrometry (MS)	900688
Ammonium hydrogen carbonate, for LC-MS LiChropur™, 50 g	5.33005
Ammonium hydroxide, OmniTrace® Ultra	AX1308-7
Formic acid, puriss. p.a., ACS reagent, reag. Ph. Eur., ≥98%	33015
Brand® Centrifuge tubes, PP, w/caps, 50 mL, Pk. 300	BR114820
Pyrex® disposable culture tubes, rimless, 10 mL, Pk. 1000	CLS9944513

Related Products

Name	Cat. No.
Methanol for UHPLC-MS LiChrosolv®	1.03726
Acetonitrile for UHPLC-MS LiChrosolv®	1.03725
Ammonia solution 25%, for HPLC LiChropur™	5.43830
Formic acid for LC-MS LiChropur™, 97.5-98.5% (T)	00940

To place an order or receive technical assistance

Order/Customer Service: SigmaAldrich.com/order

Technical Service: SigmaAldrich.com/techservice

Safety-related Information: SigmaAldrich.com/safetycenter

SigmaAldrich.com

Merck KGaA
Frankfurter Strasse 250
64293 Darmstadt, Germany

